VERIFY ALL DOCUMENTS FOR CURRENT REVISION AND PENDING CHANGES PRIOR TO EACH USE.
INIT_____ DATE_____

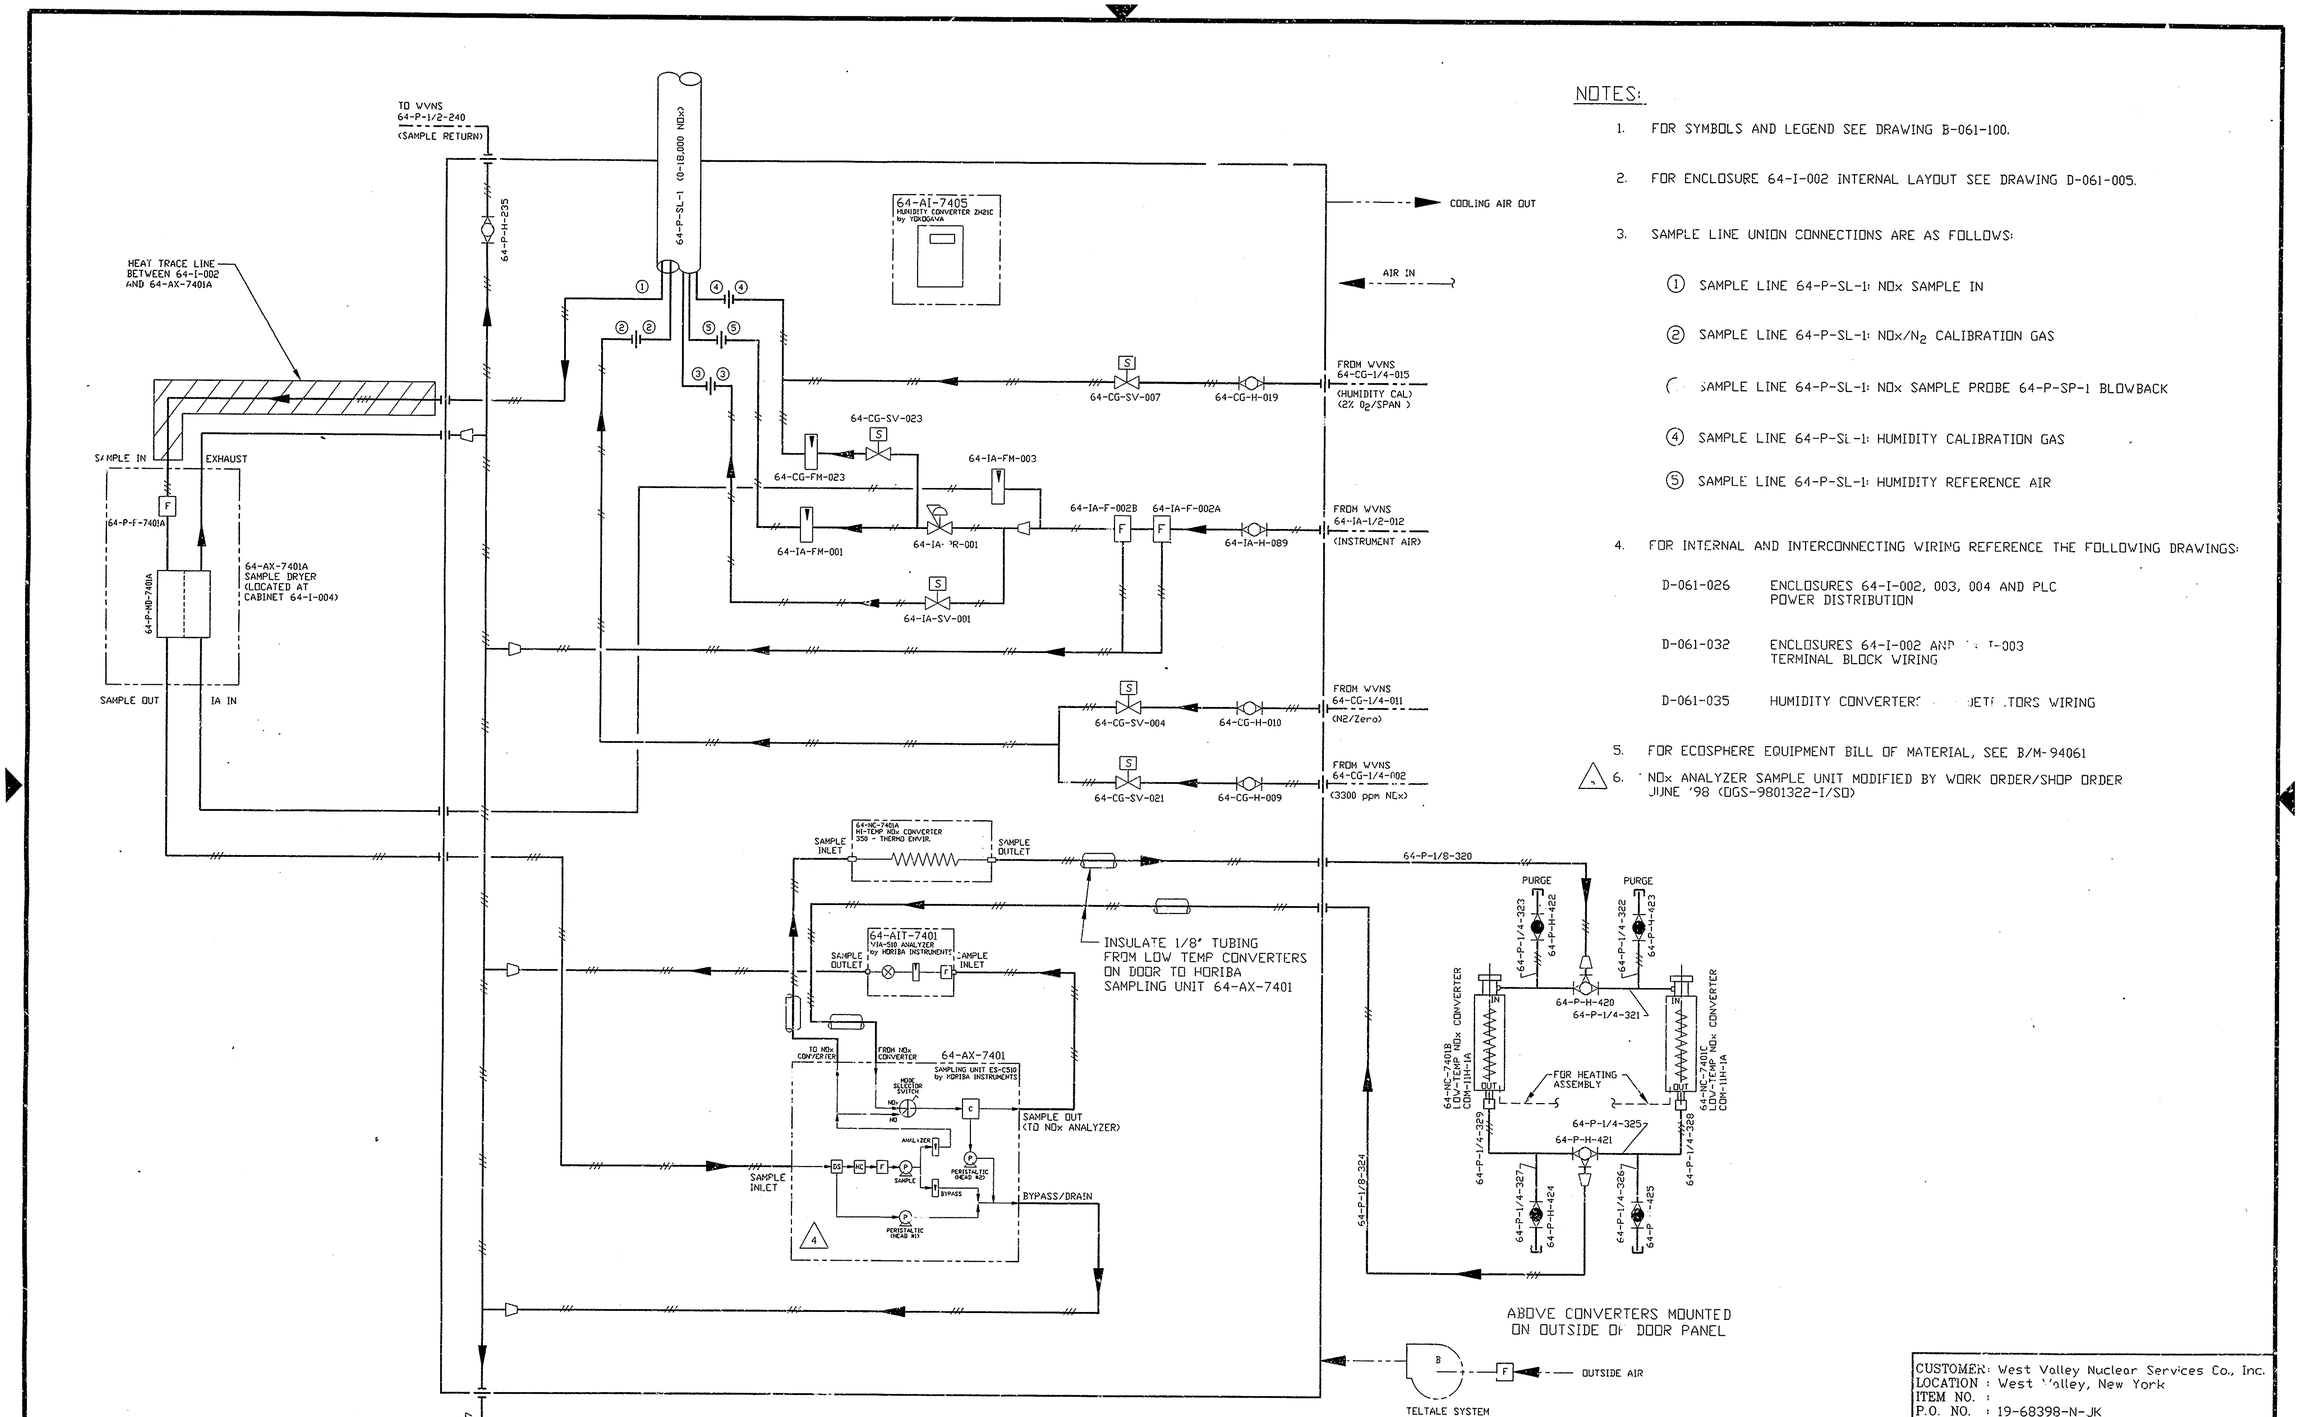

NOTES:

1. FOR SYMBOLS AND LEGEND SEE DRAWING B-061-100.
2. FOR ENCLOSURE 64-I-002 INTERNAL LAYOUT SEE DRAWING D-061-005.
3. SAMPLE LINE UNION CONNECTIONS ARE AS FOLLOWS:
   - (1) SAMPLE LINE 64-P-SL-1: NOx SAMPLE IN
   - (2) SAMPLE LINE 64-P-SL-1: NOx/N_2 CALIBRATION GAS
   - (3) SAMPLE LINE 64-P-SL-1: NOx SAMPLE PROBE 64-P-SP-1 BLOWBACK
   - (4) SAMPLE LINE 64-P-SL-1: HUMIDITY CALIBRATION GAS
   - (5) SAMPLE LINE 64-P-SL-1: HUMIDITY REFERENCE AIR
4. FOR INTERNAL AND INTERCONNECTING WIRING REFERENCE THE FOLLOWING DRAWINGS:
   - D-061-026 ENCLOSURES 64-I-002, 003, 004 AND PLC POWER DISTRIBUTION
   - D-061-032 ENCLOSURES 64-I-002 AND [illegible]-003 TERMINAL BLOCK WIRING
   - D-061-035 HUMIDITY CONVERTER[illegible] DETECTORS WIRING
5. FOR ECOSPHERE EQUIPMENT BILL OF MATERIAL, SEE B/M-94061
6. △ NOx ANALYZER SAMPLE UNIT MODIFIED BY WORK ORDER/SHOP ORDER JUNE '98 (DGS-9801322-I/SO)

LETT	ALTERATION	DATE	BY	CHK'D	APPV'D
4	ECN 11473	12/01/98	BP	DRS	
3	ECN 10191A	9/24/96	AAJ	HAB	
2	ECN TM 2358	6/24/96	JLH	DRS	
1	ECN-9752	04/22/96	SAB	HAB	JHK
0	ER#3092	10/19/95			JRH
~~D~~	~~TITLE BLOCK WAS ENCLOSURE 64-I-003~~	~~10/12/94~~	~~TDC~~		
~~A~~	~~REDRAWN ON NEW SHEET, REVISED PER AR-11 AND AS-BUILT.~~	~~9/29/94~~	~~TDC~~		

CUSTOMER: West Valley Nuclear Services Co., Inc.
LOCATION : West Valley, New York
ITEM NO. :
P.O. NO. : 19-68398-N-JK

TITLE
MELTER OFF-GAS CONTINUOUS MONITORING SYSTEM
P&ID - ENCLOSURE 64-I-002

ECOSPHERE
ENVIRONMENTAL INCORPORATED
4550 BAILEY AVENUE
BUFFALO, NEW YORK 14226-2138

JOB NO.	94-061
BY / DATE	tdc 4/25/94
SCALE	NONE
CHECKED	ALLEN
NO. SHTS	1
LATEST ALT. LETT.	
REVIEWED	CZAJKA
SHT. NO.	1
4	
APPROVED	CARR

D-061-016

ACAD FILE: D061-016